

Accredited by the Accreditation Council for Continuing Medical Education

GYN Assessment 2008

ASCP GYN Products

COURSE No.: GYN08 2


CME/CMLE Credits: 5.00

03070349 Onat Akin, MD Valikonagi Cad # 55 Istanbul, 34371 Turkey DATE: 01/28/2009

The ASCP certifies that the named individual has participated in this educational activity at the location and date indicated above and, if a physician, is awarded the indicated number of AMA PRA Category 1 credit(s)TM.

California CE Registration No. 0010 Florida Provider No. JP-0000051 7/16/2010 12:42:37PM GYN08 Sugarae Jungit

33 West Monroe, Suite 1600 Chicago, IL 60603



Accredited by the Accreditation Council for Continuing Medical Education

GYN Assessment 2010

ASCP GYN Products

COURSE No.: GYN10 2


CME/CMLE Credits: 5.00

03070349 Onat Akin, MD Valikonagi Cad # 55 Istanbul, 34371 Turkey DATE: 07/08/2010

The ASCP certifies that the named individual has participated in this educational activity at the location and date indicated above and, if a physician, is awarded the indicated number of AMA PRA Category 1 credit(s)TM.

Laborate CF Regentation No. 0010 15c.dr Panader No. 12 0000051 7/13/2010 11:28:43AM GYN10 Luzana Junach

13 West Mourne, Suste 1600 Chicago, IL 60603



Accredited by the Accreditation Council for Continuing Medical Education

GYN Assessment 2010

ASCP GYN Products


COURSE No.: GYN10 1

CME/CMLE Credits: 5.00

03070349 Onat Akin, MD Valikonagi Cad # 55 Istanbul, 34371 Turkey DATE: 03/05/2010

The ASCP certifies that the named individual has participated in this educational activity at the location and date indicated above and, if a physician, is awarded the indicated number of AMA PRA Category 1 credit(s)TM.

California CE Registration No. 0010 Florida Provider No. JP-0000051 7/13/2010 11:28:43AM GYN10 Sugaran Jingib 33 West Monroe, Suite 1600 Chicago, II. 60603



Accredited by the Accreditation Council for Continuing Medical Education

GYN Assessment 2008

ASCP GYN Products

COURSE No.: GYN08 3

CME/CMLE Credits: 5.00


03070349 Onat Akin, MD Valikonagi Cad # 55 Istanbul, 34371 Turkey DATE: 06/03/2009

The ASCP certifies that the named individual has participated in this educational activity at the location and date indicated above and, if a physician, is awarded the indicated number of AMA PRA Category 1 credit(s)***M.

California CE Registration No. 0010 Florida Provider No. JP-0000051

7/16/2010 12:42:37PM GYN08

Sugaran Zingaib 33 West Monroe, Suite 1600 Chicago, II. 60603



Accredited by the Accreditation Council for Continuing Medical Education

GYN Assessment 2008

ASCP GYN Products

COURSE No.: GYN08 1


CME/CMLE Credits: 5.00

03070349 Onat Akin, MD Valikonagi Cad # 55 Istanbul, 34371 Turkey DATE: 09/23/2008

The ASCP certifies that the named individual has participated in this educational activity at the location and date indicated above and, if a physician, is awarded the indicated number of AMA PRA Category 1 credit(s)TM. 01575 PATOMED LABORATORY
M42-1 ASCP GYN Assessment #M42-1
Region: I

Regional Comparison

Summary of Laboratories' Performances on Routine Cases in comparison to all regions with Labs reviewing the same cases

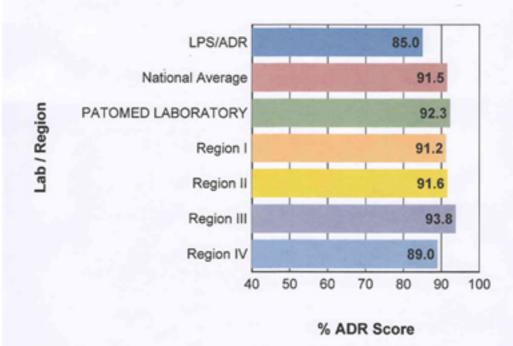

Program Information

M42-1 ASCP GYN Assessment #M42-1 Program Makeup: Routine Ceses: 13 Moderate Ceses: 1 Difficut Desex: 1

1-1

GLOSSARY OF TERMS

LPS: Lab Performance Standard: a percentage of correct responses designated as a baseline of performance for laboratories


ACR: Acceptable Diagnostic Range: a range of acceptable responses including the Target DX plus minor deviations above and/or below 01575 PATOMED LABORATORY

M26-2 ASCP GYN Assessment #M26-2

Region: I

Regional Comparison

Summary of Laboratories' Performances on Routine Cases in comparison to all regions with Labs reviewing the same cases

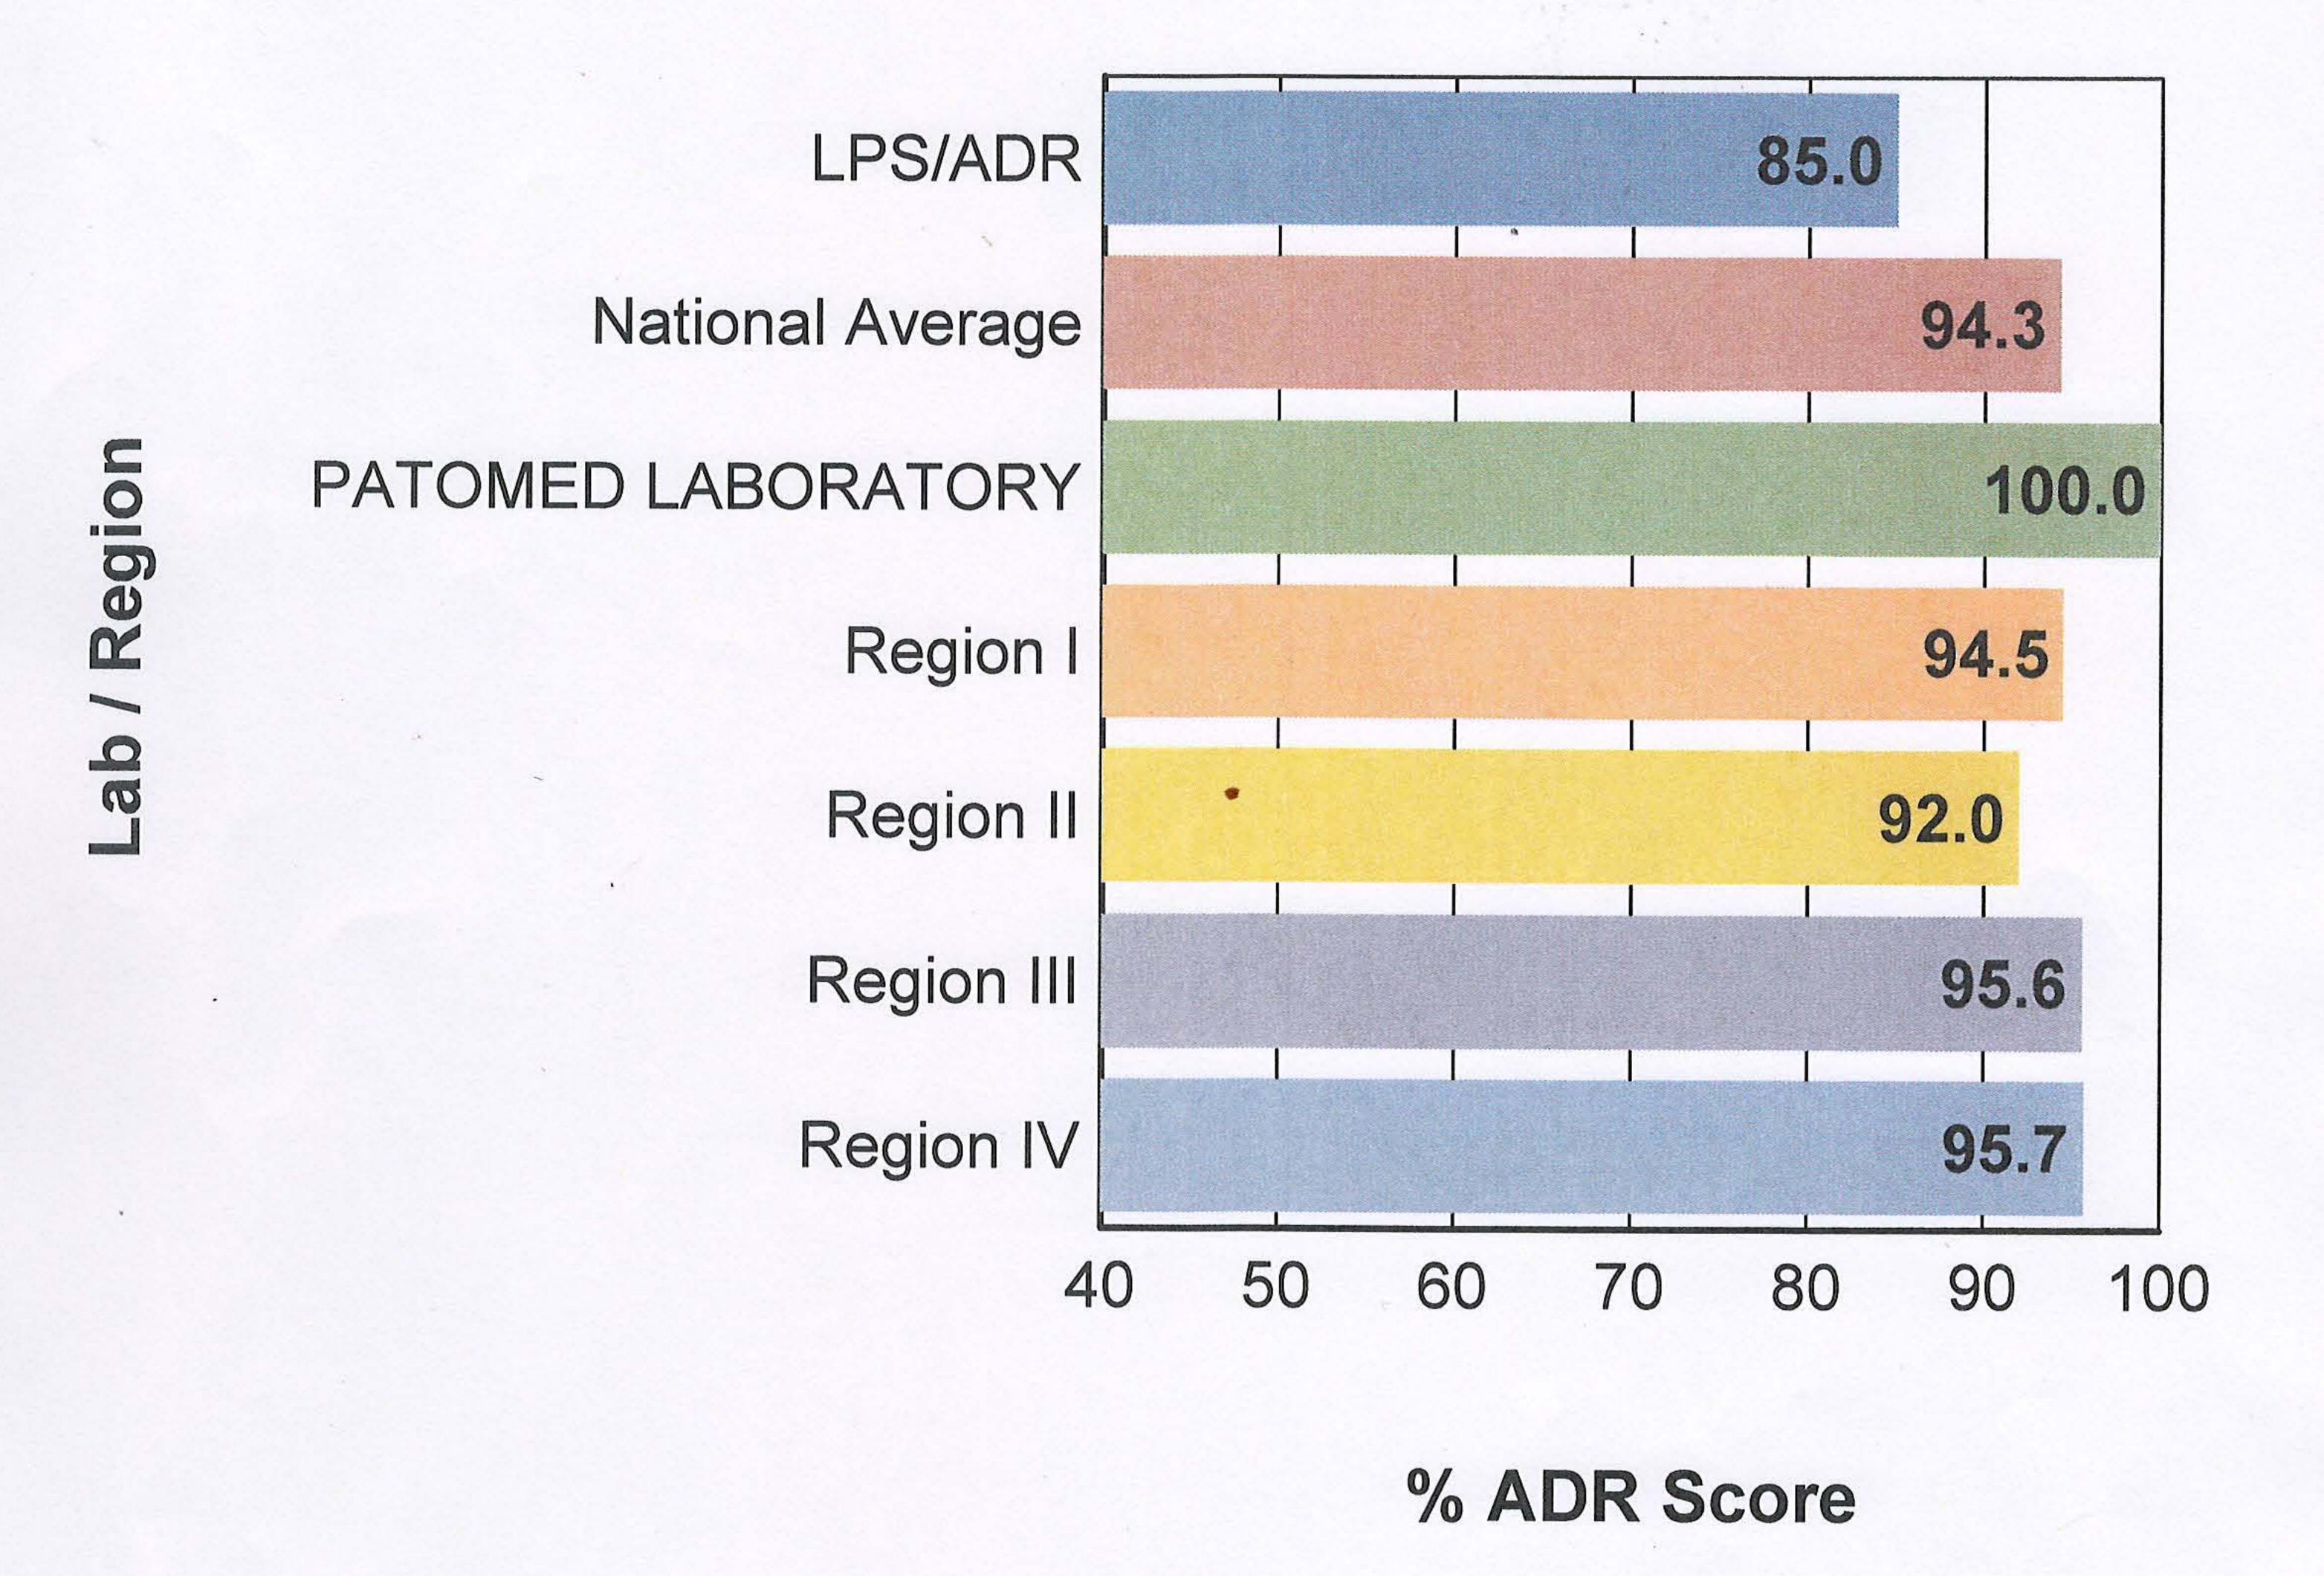

Program Information

M26-2 ASCP GYN Assessment #M26-2

Program Makeup: Routine Cases: 12

Moderate Cases: 2 Difficult Dases: 1

GLOSSARY OF TERMS

LPS: Lab Performance Standard; a percentage of correct responses designated as a baseline of performance for laboratories

ADR: Acceptable Diagnostic Range; a range of acceptable responses including the Target DX plus minor deviations above and/or below